

HPLC Analysis Report

Sample: Dapoxetine HCL

Buffer A: 0.04% TFA in 100% water(v/v)

Buffer B: 0.04% TFA in 100% acetonitrile (v/v)


Gradient: 10-80% Buffer B in 25 min then 100% Buffer B for 5 min.

Flow: 1ml/min Wavelength:220nm

Column: Alltima C18,4.6*250mm,5um

Date: May 13, 2014

Chromatogram

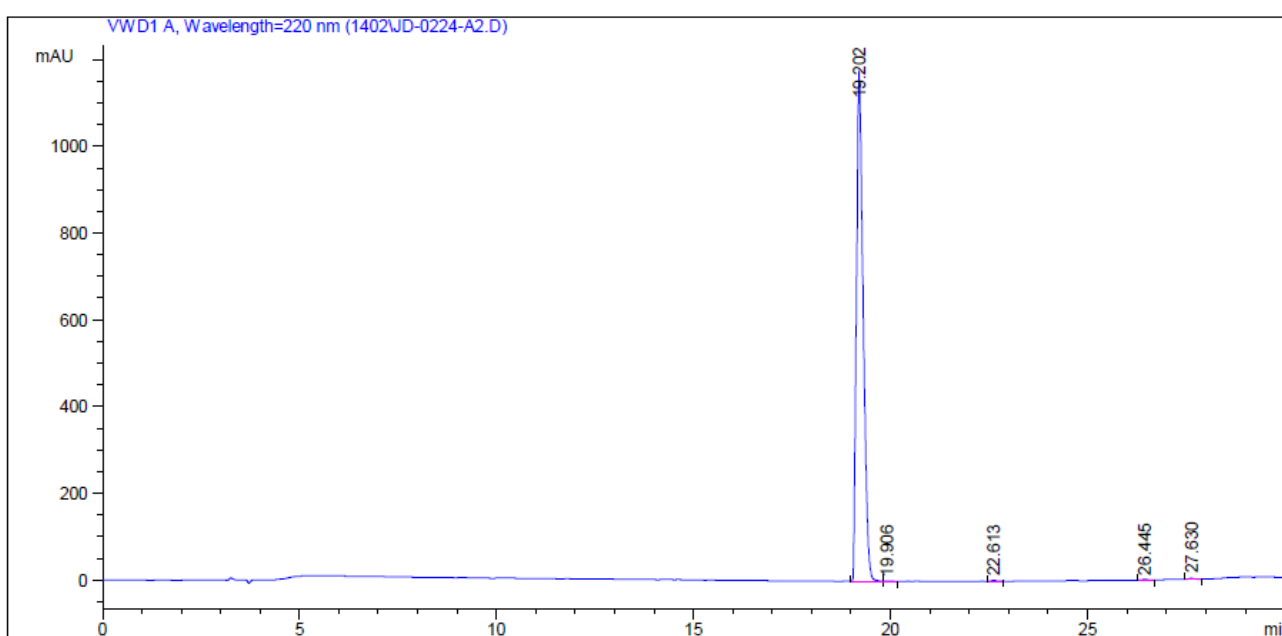

Peak#	RetTime(Min)	Width(Min)	Area(mAU*s)	Height(mAU)	Area(%)
1	19.202	0.1705	1.39599e4	1176.28748	99.4169
2	19.906	0.1424	11.69364	1.22031	0.0833
3	22.613	0.1538	18.49657	1.77209	0.1317
4	26.445	0.1711	13.89599	1.20339	0.0990
5	27.630	0.1679	37.78530	3.28075	0.2691
Totals			1.40417e4	1183.76401	100