

KI0115 HPLC Analysis Report

Sample: Ganetespib

Sample ID: KI0115

Buffer A: 0.1% TFA in 100% water (v/v)


Buffer B: 0.1% TFA in 80% acetonitrile + 20% water (v/v)

Gradient: 51-71% Buffer B in 20min

Flow: 1ml/min Wavelength: 220nm

Column: Venusil C18 5um 4.6*250mm

Chromatogram

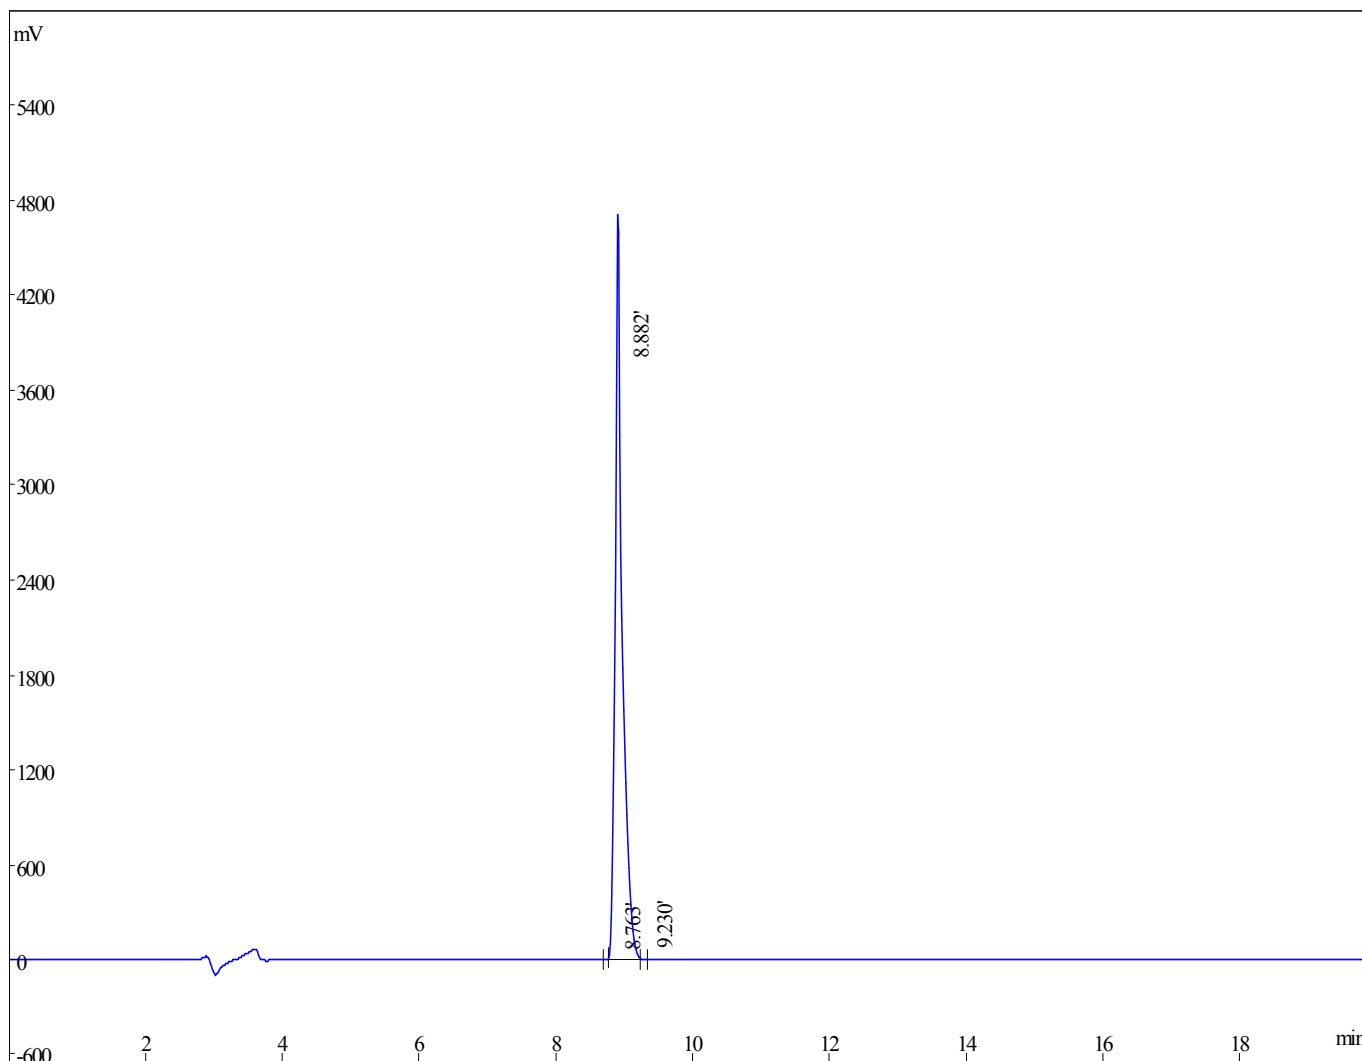

| Signal | Peak# | RT (min) | Area% | Area (mAU*s) | Height (mAU) |
|--------------|-------|----------|------------|-----------------|----------------|
| | 1 | 8.950 | 0.06076 | 6741 | 6662 |
| | 2 | 9.148 | 99.9 | 11082947 | 1120606 |
| | 3 | 9.455 | 0.03777 | 4190 | 2656 |
| Total | | | 100 | 11093878 | 1129924 |