

HPLC Analysis Report

Sample: Pramipexole HCl

Buffer A: 0.04% TFA in 100% water(v/v)

Buffer B: 0.04% TFA in 100% acetonitrile (v/v)


Gradient: 0-30% Buffer B in 25 min

Flow: 1ml/min Wavelength:220nm

Column: Alltima C18,4.6*250mm,5um

Date: Jan. 9, 2014

Chromatogram

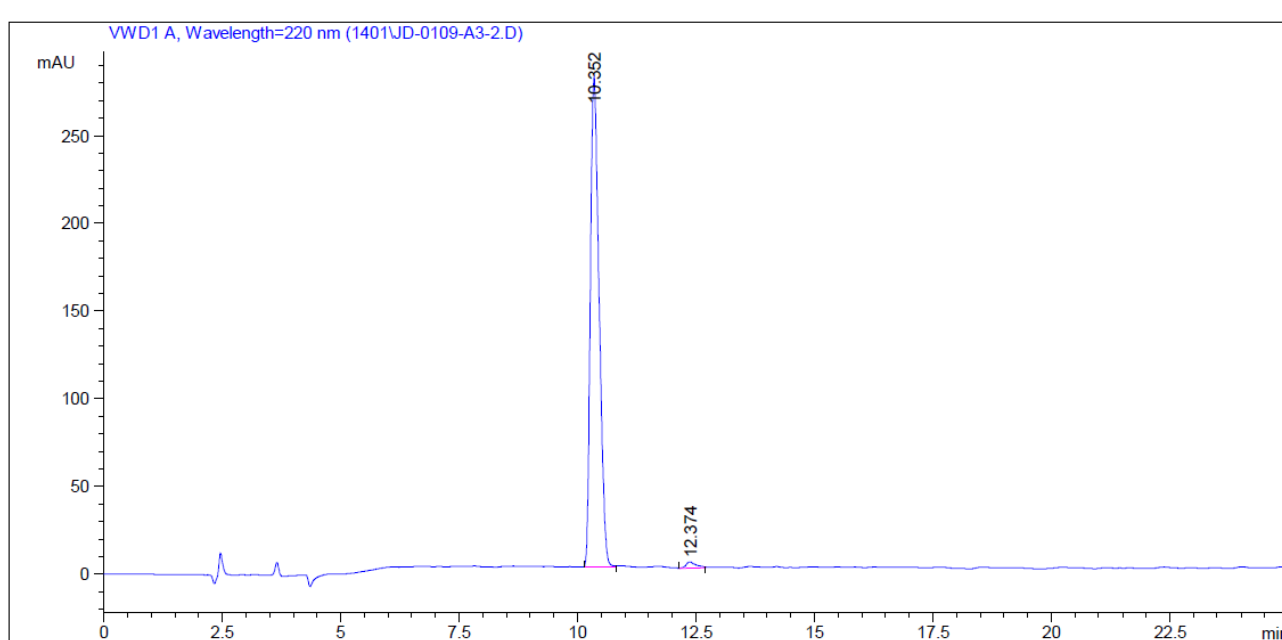

Peak#	RetTime(Min)	Width(Min)	Area(mAU*s)	Height(mAU)	Area(%)
1	10.352	0.2024	3571.41943	277.76041	98.6071
2	12.374	0.2201	50.44722	3.39133	1.3929
Totals			3621.86666	281.15174	100